Quick Guide

elsa™ mein Tourniquet
heidi™ mein Tourniquet
ATMOS MedizinTechnik

Step 1:

Connect cuff AFTER the self-test



Step 2:

Choose extremity of blood arrest

Choose the extremity (arm/leg) on the 'patient' symbol and confirm.

Step 3:

Start of blood arrest application


Start the blood arrest by pressing the 'air pump' symbol.

Step 4:

End of blood arrest application

End the blood arrest by pressing the 'deflate' symbol.

Press the 'cancel' symbol to go to the history.

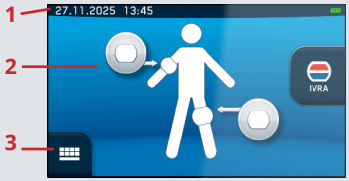

1 Status line
(date, time, error message, service, mains power, battery)

2 Control panel

3 Menu

During the surgery:

- Pressure can be regulated with the 'plus/minus' symbol.
- Check the blood arrest duration with the 'countdown info' symbol.

Once the countdown has finished, you can set it again.



Technical specifications subject to change; printing errors and omissions excepted.

⚠ This Quick Guide does not replace the instructions for use.

Consult the instructions for use!

Warnings and errors

Code	Cause
Notification	
	Battery is defective Battery fuse is incorrectly inserted
Warnings	
W 301	Recording
W 311	Safety check required
W 321	Battery nearly empty
W 360	Battery empty
Errors	
E 99	Device check not passed
E 120 / E 420	Internal memory error
E 140	Pressure measurement inconsistent
E 145	Valve switching malfunction
E 155 / E 555 / E 655	Compressor malfunction
E 530	No cuff attached
E 645	Malfunction of the switching and regulating behaviour of the valves
E 650	Leak message
E 660	Battery empty
E 665	Overly high pressure in the cuff
E 875	Internal power supply error
E 880	Safety message in pressure measurement
E 890	Software error
E 895	Overtemperature message (>65 °C)